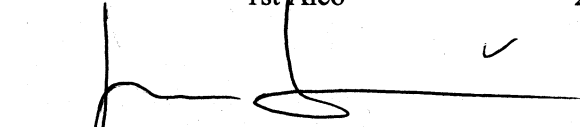# VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument
State of Alaska

JUN 2 4 2009

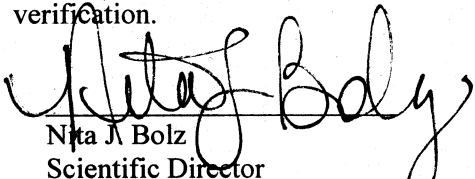*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

A

DataMaster cdm S/N _____ 130569 _____ ✓

Supervisor/Operator Performing the Verification Procedure:

Name _____ **John Hodges** _____ ID # _____ **2999** _____ Date _____ **6/19/2009** ✓

Agency _____ **Cordova Police Department** _____ Phone # _____ **424-6100** _____

Instrument Location _____ **Cordova Police Department** _____

B

Alco S/N _____ **X124634** ✓ Target Value _____ **0.078** ✓ High Pressure **750psi**

Alco Test Value Average _____ **0.080** ✓ _____ **0.080** ✓
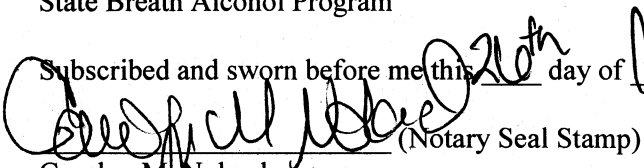
1st Alco   2nd Alco

Signature _____

(OVER)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

(Do Not write in the area below)

(1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.

(2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.

(3) I am the Scientific Director of the State Breath Alcohol Program.

(4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.

(5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 24th day of June 2009.

(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

BT9 03/00

VERIFICATION OF CALIBRATION REPORT

Of Data Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statedwide Breath Alcohol Program

---

DataMaster cdm S/N   130569 ✓

(CONTINUED FROM FRONT PAGE)

C   TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

```
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JUNE 19, 2009

OPERATOR'S NAME:
  HODGES, JOHN
OPERATOR'S NUMBER: 2999
SUBJECT'S LAST NAME:
  VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
  X
O.L. #: X
DEPT/AGENCY: CDV1
CASE/REPORT: X
TEST TYPE: V
ALCO TARGET VALUE: .078   ✓
ALCO S/N: X124634

    --- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.88 in  ✓
ALCO TARGET       .077      21:18
BLANK TEST        .000      21:20
INTERNAL STANDARD VERIFIED  21:20
ALCO TV 29.88 in  .080  ✓   21:20
BLANK TEST        .000      21:21
SUBJECT SAMPLE    .000      21:22
BLANK TEST        .000      21:23
ALCO TV 29.88 in  .080  ✓   21:23
BLANK TEST        .000      21:24
```

(handwritten: BMB 6/25/09)
(handwritten: 6-19-09)
(handwritten: BMB 6/25/09)

DIAGNOSTIC CHECK

```
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130569

JUNE 19, 2009   ✓
TIME 21:26

    --- DIAGNOSTIC CHECK ---

COMPUTER:          OKAY

PROGRAM:           OKAY

SOFTWARE DATE:     02/20/01

HEATERS
SAMPLE CHAMBER:    49c
BREATH TUBE:       42c

BAROMETER:         29.88 in

FLOW DETECTOR:     OKAY

PUMP
HIGH SPEED:        OKAY

DETECTOR:          OKAY

FILTERS:           OKAY

QUARTZ STANDARD:   OKAY

CALIBRATION:       OKAY

        PRINTER TEST
!"#$%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmno
pqrstuvwxyz{|}~
```

BT9 03/00